GETINGE

GETINGE 88-SERIES
PROGRAM EUROPE
5027915-21,-23,-24,-26,-27,-28

SEV0738065-

GETINGE

HOSPITAL A_0 3000 (90 °C - 5 MIN)

This program sheet applies to 5024374-21,-23,-24,-26,-27.

Programs	Program selection button					Type of goods
5024374	**-21**	**-23**	**-24**	**-26**	**-27**	
POWER CLEAN	P1		P1	P1		Very dirty instruments
OP-SHORT-D	P2		P2	P2		Instruments, tubular instruments
OP-D	P3		P3	P3		Instruments, tubular instruments
OP-LONG-D	P4		P4	P4		Very dirty instruments
AN-D	P5	P5	P5	P5	P5	Anaesthesia tubing
ENZYM-SHORT-D			P8*			Instruments, tubular instruments
ENZYM-D			P9*			Instruments, tubular instruments
OP-SHORT-D-3		P2			P2	Instruments, tubular instruments (Inst. milk)
OP-D-3		P3			P3	Instruments, tubular instruments (Inst. milk)
OP-LONG-D-3		P4			P4	Very dirty instruments (Inst. milk)
OP-BGA (A+B)-D-3		P7*	P7*		P7*	Circulation goods, instruments. (90 °C - 10 min) (Inst. milk)
OS-CHEM-D			P6	P8*	P8*	OP-shoes
OP-BGA (A+B)-D	P7*			P7*		Circulation goods, instruments. (90 °C - 10 min)
AN-BGA (A+B)-D	P6	P6		P6	P6	Anaesthesia tubing. (90 °C - 10 min)
DRYING						Drying
DELIMING	P12*	P12*	P12*	P12*	P12*	DeLIMEING of chamber, inserts washer arms and washer vanes. Dose 200 ml Neudish BU (sold by Dr.Weigert) into the wash chamber. **NOTE: Do not have any goods in the machine with this program. It is only for descaling the machine.**
COMPLETE DRAIN	P17*	P17*	P17*	P17*	P17*	Complete drain
DOOR TEST	P14*	P14*	P14*	P14*	P14*	Door test
DISINF PROCESS TANK	P15*	P15*	P15*	P15*	P15*	Disinfection of process tank

*** For choosing this program, see instructions for use.**

Process times may vary depending on whether the machine is equipped with steam or electrical heating.
The temperature of the incoming water also affects process times.

<Doc_SUB><Doc_502791500><Rel_A><Lang_GB>

GETINGE

POWER CLEAN

A=120ml

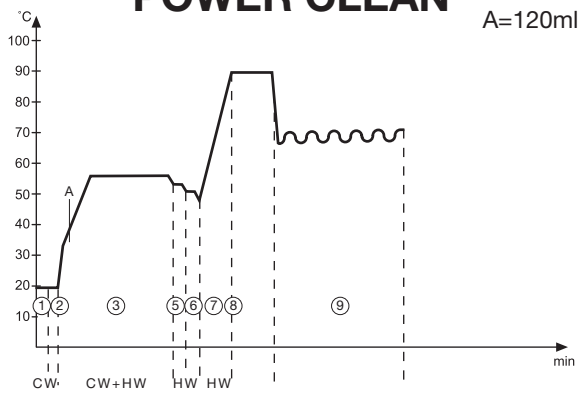

OP-SHORT-D

A=120ml
B= 40ml

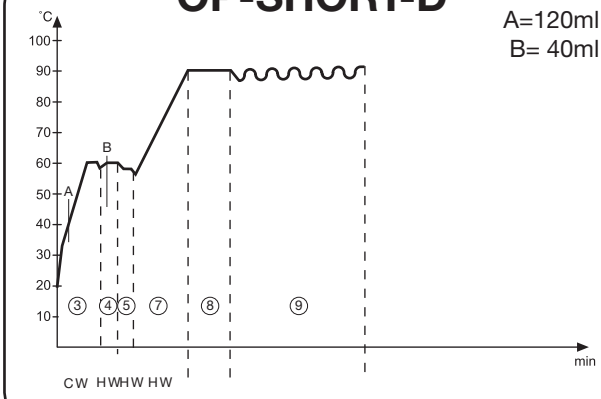

OP-D

A=120ml
B= 40ml

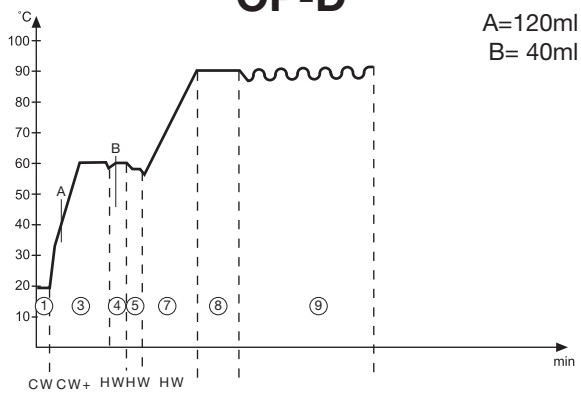

OP-LONG-D

A=120ml
B= 40ml

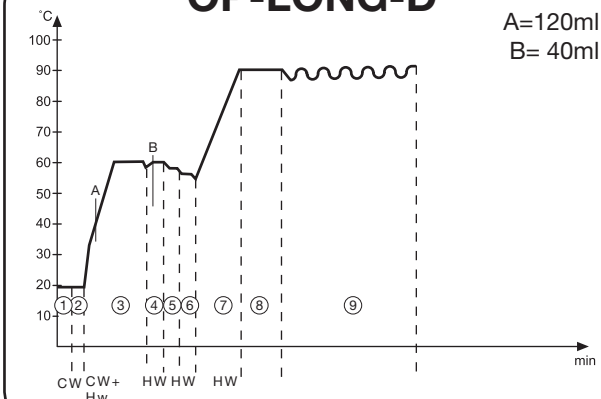

AN-D

A=120ml
B= 40ml

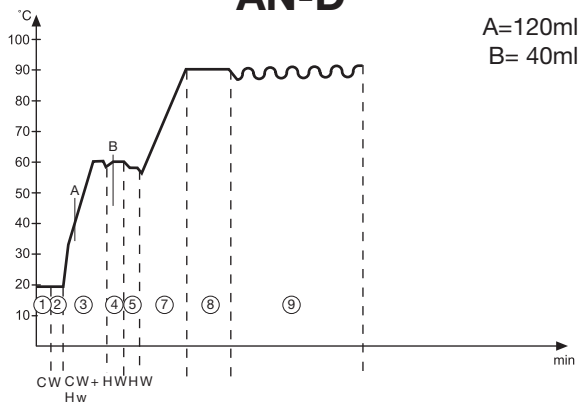

ENZYM-SHORT-D

D= 240ml

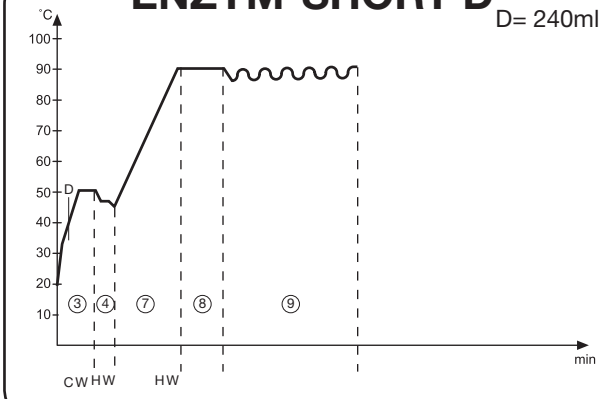

NOTE: To choose the recommended agent, see under Agent in the user instructuions.
The amount of agent are basic setting at delivery.

Process times may vary depending on whether the machine is equipped with steam or electrical heating.
The temperature of the incoming water also affects process times.

<Doc_SUB><Doc_502791500><Rel_A><Lang_GB>

GETINGE

ENZYM-D

D= 240ml

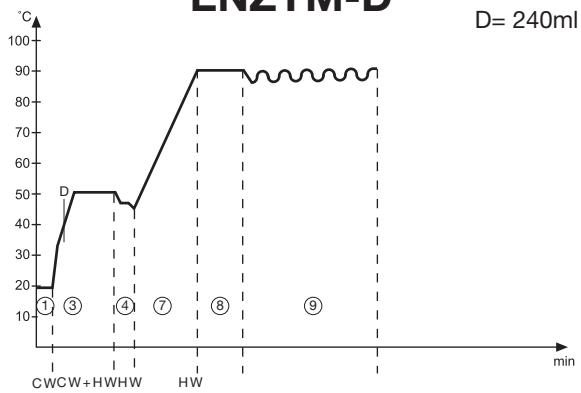

OP-SHORT-D-3

A=120ml
B= 40ml
C= 30ml

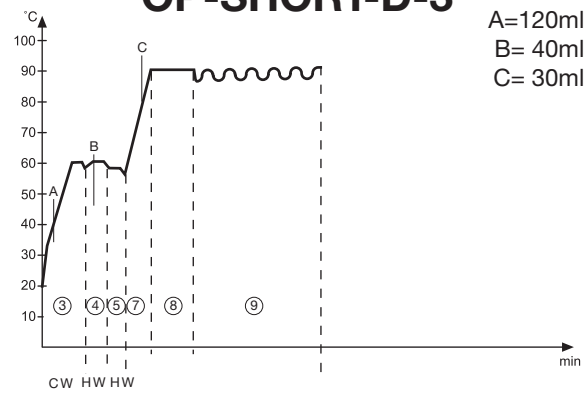

OP-D-3

A=120ml
B= 40ml
C= 30ml

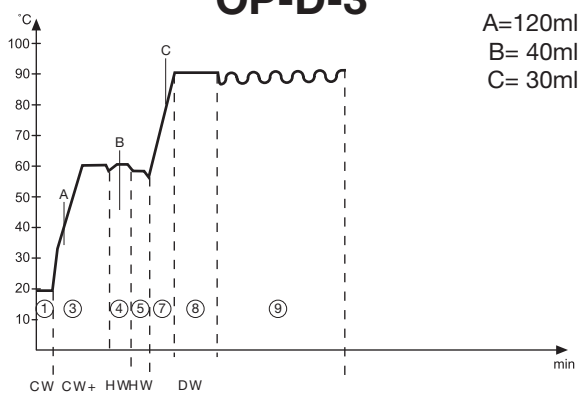

OP-LONG-D-3

A=120ml
B= 40ml
C= 30ml

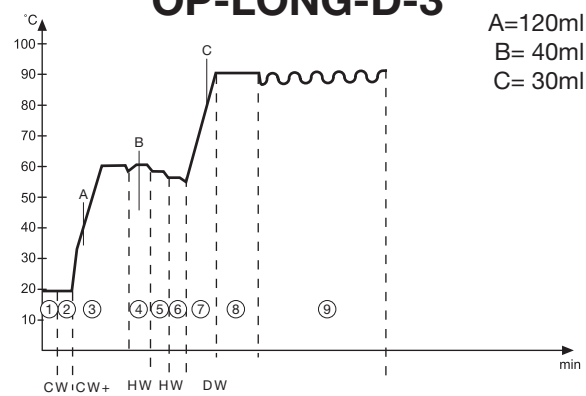

OP-BGA (A+B)-D-3

A=120ml
B= 40ml
C= 30ml

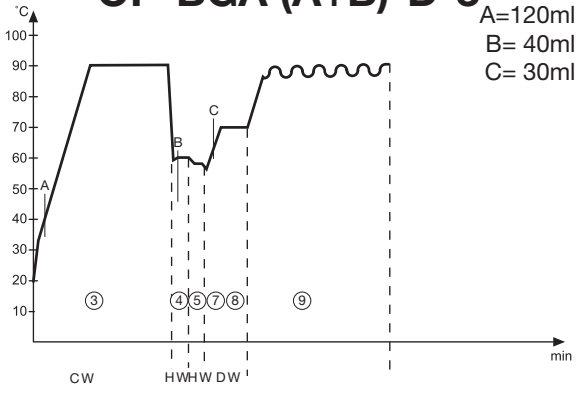

Program phases

1	Pre-rinse 1	A	Alkaline detergent
2	Pre-rinse 2	B	Neutralizing
3	Wash	C	Instrument milk (option) When dosing instrument milk, rinse-aid is not dosed.
4	Neutralize	D	Enzym
5	Post-rinse 1	E	Chemical disinfection
6	Post-rinse 2		
7	Final rinse		
8	Disinfection		
9	Drying		

NOTE: To choose the recommended agent, see under Agent in the user instructuions.
The amount of agent are basic setting at delivery.

Process times may vary depending on whether the machine is equipped with steam or electrical heating.
The temperature of the incoming water also affects process times.

<Doc_SUB><Doc_502791500><Rel_A><Lang_GB>

GETINGE

OS-CHEM-D

A= 120ml
E= 400ml

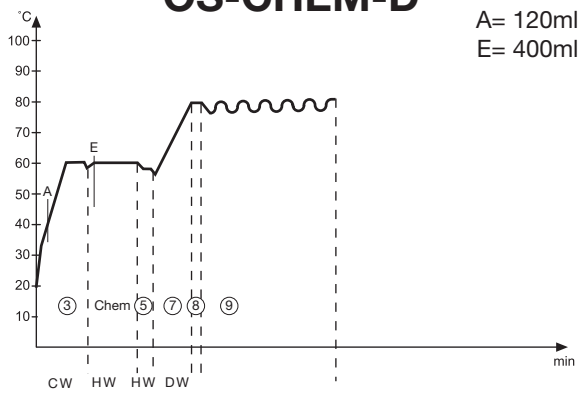

OP-BGA (A+B)-D

A= 120ml
B= 40ml

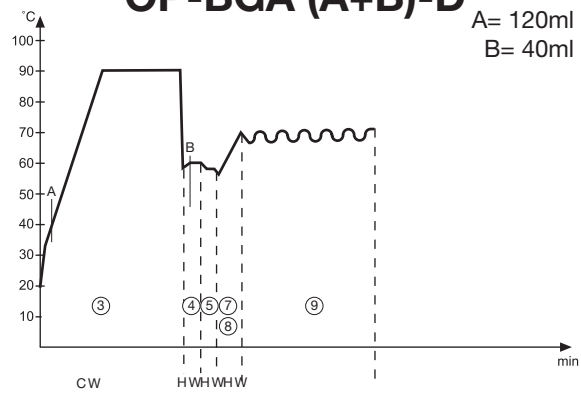

AN-BGA (A+B)-D

A= 120ml
B= 40ml

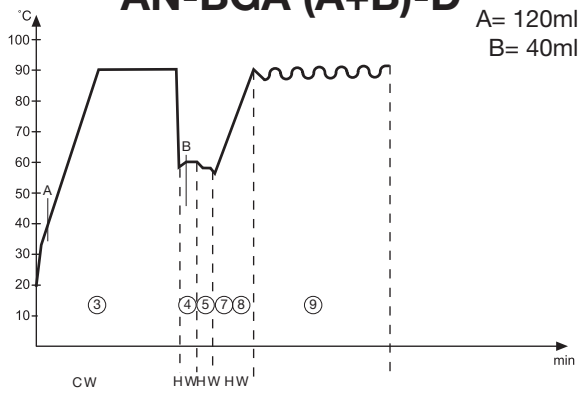

DRYING

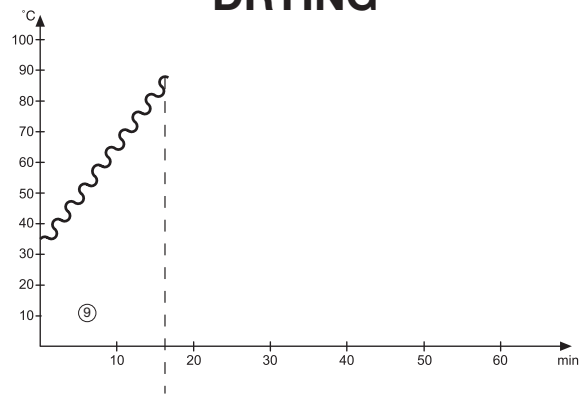

DELIMEING

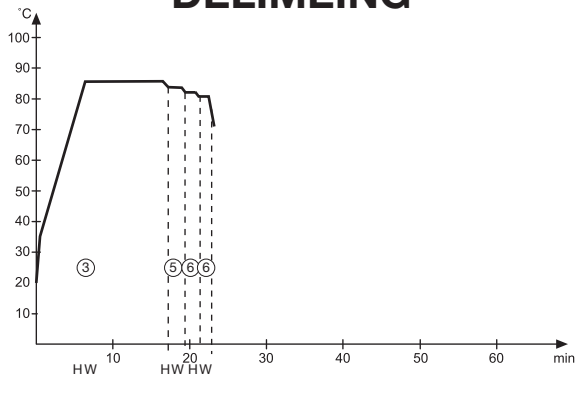

Program phases

1	Pre-rinse 1	A	Alkaline detergent
2	Pre-rinse 2	B	Neutralizing
3	Wash	C	Instrument milk (option) When dosing instrument milk, rinse-aid is not dosed.
4	Neutralize	D	Enzym
5	Post-rinse 1	E	Chemical disinfection
6	Post-rinse 2		
7	Final rinse		
8	Disinfection		
9	Drying		

NOTE: To choose the recommended agent, see under Agent in the user instructuions.
The amount of agent are basic setting at delivery.

Process times may vary depending on whether the machine is equipped with steam or electrical heating.
The temperature of the incoming water also affects process times.

<Doc_SUB><Doc_502791500><Rel_A><Lang_GB>

GETINGE

LIFE SCEINCE

This program sheet applies to 5024374-28.

Programs	Program selection button	Type of goods
LAB-SHORT-D	P1	Slightly dirty labgods
LAB-D	P2	Labgods
LAB-LONG-D	P3	Very dirty instruments
TEST TUBES-D	P4	Test tubes
PIPETTES-D	P5	Pipettes

Process times may vary depending on whether the machine is equipped with steam or electrical heating.
The temperature of the incoming water also affects process times.

LAB-SHORT-D

A=120ml
B= 40ml

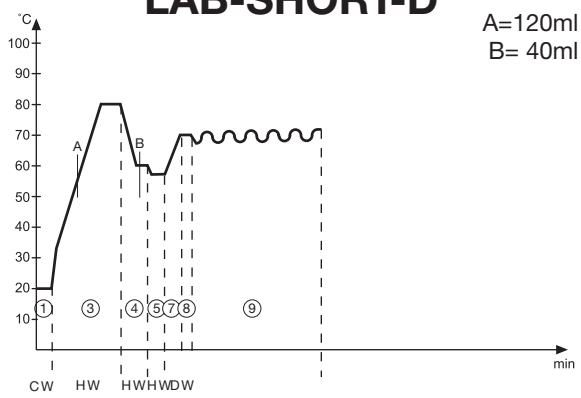

LAB-D

A=120ml
B= 40ml

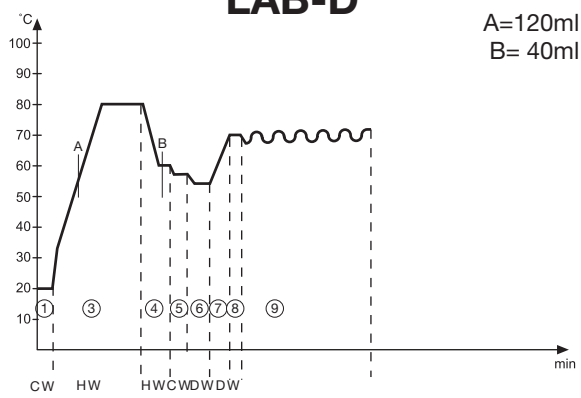

LAB-LONG-D

A=120ml
B= 40ml

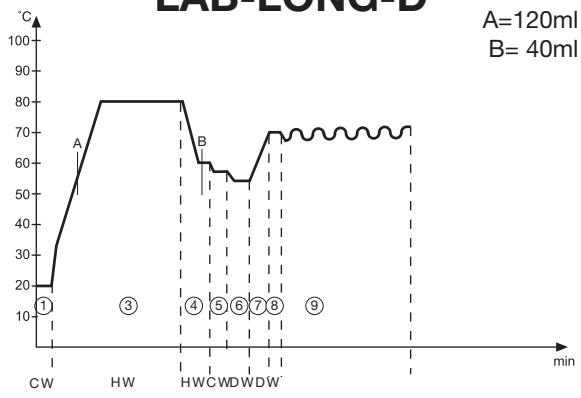

Program phases

1 Pre-rinse 1
2 Pre-rinse 2
3 Wash
4 Neutralize
5 Post-rinse 1
6 Post-rinse 2
7 Final rinse
8 Disinfection
9 Drying

A Alkaline detergent
B Neutralizing
C Instrument milk (option) When dosing instrument milk, rinse-aid is not dosed.
D Enzym
E Chemical disinfection

NOTE: To choose the recommended agent, see under Agent in the user instructuions.
The amount of agent are basic setting at delivery.

Process times may vary depending on whether the machine is equipped with steam or electrical heating.
The temperature of the incoming water also affects process times.

<Doc_SUB><Doc_502791500><Rel_A><Lang_GB>

GETINGE

TEST TUBES-D

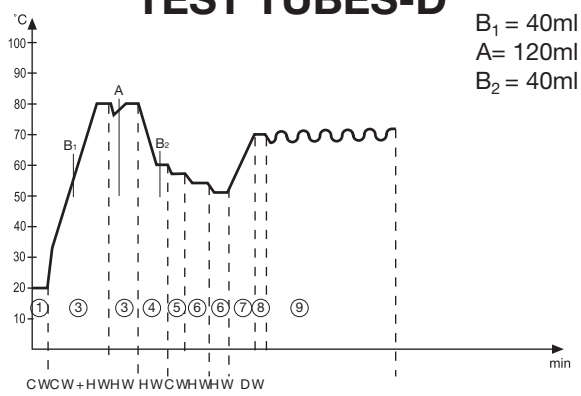

B_1 = 40ml
A= 120ml
B_2 = 40ml

PIPETTES-D

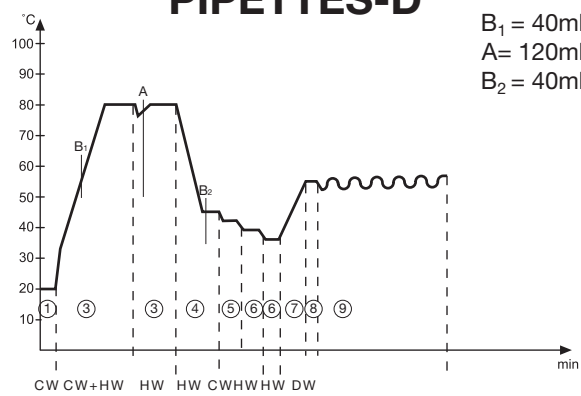

B_1 = 40ml
A= 120ml
B_2 = 40ml

Program phases

1	Pre-rinse 1	A	Alkaline detergent
2	Pre-rinse 2	B	Neutralizing
3	Wash	C	Instrument milk (option) When dosing instrument milk, rinse-aid is not dosed.
4	Neutralize	D	Enzym
5	Post-rinse 1	E	Chemical disinfection
6	Post-rinse 2		
7	Final rinse		
8	Disinfection		
9	Drying		

NOTE: To choose the recommended agent, see under Agent in the user instructuions.
The amount of agent are basic setting at delivery.

Process times may vary depending on whether the machine is equipped with steam or electrical heating.
The temperature of the incoming water also affects process times.

<Doc_SUB><Doc_502791500><Rel_A><Lang_GB>

Australia
Getinge Australia Pty Ltd
154 Lytton Road
Bulimba Qld 4171
info@getinge.com.au
Phone: +61-733 956 311

Belgium
Getinge NV
Nijverheidsstraat 2
BE-2160 Wommelgem
info@getinge.be
Phone: +32-33542865

Canada
Getinge Canada Ltd
1575 South Gateway Road,
Unit C
Mississauga Ontario
L4W 5J1
info@getingecastle.ca
Phone: +1-905 629 8777

China
Getinge (Suzhou) Co. Ltd
Rm. 720, 7/F, Century Financial Tower
No. 1,
Su Hua Road, Suzhou Industrial Park,
Suzhou,
Jiangsu Province
Phone: + (86512) 67621587,
67621589, 67611591

Getinge Shanghai Trading Co. Ltd
Unit C, 8/F, Luck Plaza,
300 Xuanhua Road, Shanghai
P.R. China
info@getinge.com.cn
www.getinge.com/cn
Phone: +86 21 5208 1122

Denmark
Getinge Danmark A/S
Firskovvej 23
DK-2800 Lyngby
getinge.danmark@getinge.com
www.getinge.dk
Phone: +45-45 93 27 27

Finland
Getinge Finland Ab
Hallonnäsgatan 23A,
FI-00210 Helsinki
getinge@getinge.fi
Phone: +358-968 241 20

France
Getinge France SAS
BP 49, avenue du Canada
ZA de Courtaboeuf
Les Ulis, FR-91942
getinge.france@getinge.fr
Phone: +33-1 64 86 89 00

Germany
Getinge Van Dijk
Medizintechnik GmbH
Postfach 1125
Boekholter Weg 1B
DE-47628 Straelen
info@getingevandijk.de
Phone: +49-283 491 330

Italy
Getinge S.p.A.
Via dei Buonvisi 61/D
IT-00148 Roma
info@getinge.it
www.getinge.com/it
Phone: +39-06656631

Netherlands
Getinge B.V.
Fruitenniersstraat 27, Zwijndrecht
Postbus 1004
NL-3330 CA Zwijndrecht
info@getinge.nl
Phone: +31-78 610 24 33

Norway
Getinge Norge AS
Enebakk vn.117.
N-0680 Oslo
info@getinge.no
www.getinge.com/no
Phone: +47-23 03 52 00

Poland
Getinge Poland
Ul. Lirowa 27
02-387 Warszawa
office@getinge.pl
Phone: +48-22 882 06 26

Singapore
Getinge International Far East Pte.
Ltd.
20 Bendemeer Road,
#06-02, Cyberhub Building
Singapore, SG-339914
Phone: + 65 6396 7298

South Africa
Getinge South Africa (Pty) Ltd
P O Box 48492
Hercules
Pretoria SA 0002
getinge@mweb.co.za
Phone: +27-123 721 370

Spain
Getinge Iberica SL
P.E. San Fernando, Avda. Castilla 2,
Edif. Francia 1era planta
San Fernando de Henares
Madrid ES-28830
administracion@getinge.es
www.getinge.com
Phone: + 34-916 78 26 26

Sweden
Getinge International AB
P O Box 69
SE-310 44 Getinge
info@getinge.com
Phone: +46-35 15 55 00

Switzerland
Getinge ALFA AG
Weidenweg 17
4310 Rheinfelden
info@alfa.ag
www.getingealfa.ch
Phone: +41-61 836 15 15

United Kingdom
Getinge UK Ltd
Orchard Way
Calladine Park
Sutton-In-Ashfield
Notts NG 17 1JU
sales@getinge.co.uk
Phone: +44-1623510033

USA
Getinge USA Inc.
1777 East Henrietta Road
Rochester, NY 14623-3133
info@getingeusa.com
www.getingeusa.com
Phone: +1-585 475 9040

GETINGE
www.getinge.com